



**Total Prostate Specific Antigen (PSA) Test System**  
**Product Code: 2125-300**

**1.0 INTRODUCTION**

**Intended Use: The Quantitative Determination of Total Prostate Specific Antigen (PSA) Concentration in Human Serum by a Microplate Enzyme Immunoassay, Colorimetric**

**2.0 SUMMARY AND EXPLANATION OF THE TEST**

Prostate Specific Antigen (PSA) is a serine protease with chymotrypsin-like activity.<sup>1,2</sup> The protein is a single chain glycoprotein with a molecular weight of 28.4 kDA.<sup>3</sup> PSA derives its name from the observation that it is a normal antigen of the prostate, but is not found in any other normal or malignant tissue.

PSA is found in benign, malignant and metastatic prostate cancer. Since prostate cancer is the second most prevalent form of male malignancy, the detection of elevated PSA levels plays an important role in the early diagnosis. Serum PSA levels have been found to be more useful than prostatic acid phosphatase (PAP) in the diagnosis and management of patients due to increased sensitivity.<sup>4</sup>

In this method, PSA calibrator, patient specimen or control is first added to a streptavidin coated well. Biotinylated monoclonal and enzyme labeled antibodies (directed against distinct and different epitopes of PSA) are added and the reactants mixed. Reaction between the various PSA antibodies and native PSA forms a sandwich complex that binds with the streptavidin coated to the well.

After the completion of the required incubation period, the enzyme-PSA antibody bound conjugate is separated from the unbound enzyme-PSA conjugate by aspiration or decantation. The activity of the enzyme present on the surface of the well is quantitated by reaction with a suitable substrate to produce color.


The employment of several serum references of known total prostate specific antigen (PSA) levels permits the construction of a dose response curve of activity and concentration. From comparison to the dose response curve, an unknown specimen's activity can be correlated with PSA concentration.

**3.0 PRINCIPLE**

**Immunoenzymometric assay (TYPE 3):**


The essential reagents required for an immunoenzymometric assay include high affinity and specificity antibodies (enzyme and immobilized), with different and distinct epitope recognition, in excess, and native antigen. In this procedure, the immobilization takes place during the assay at the surface of a microplate well through the interaction of streptavidin coated on the well and exogenously added biotinylated monoclonal anti-PSA antibody. Upon mixing monoclonal biotinylated antibody, the enzyme-labeled antibody and a serum containing the native antigen, reaction results between the native antigen and the antibodies,

without competition or steric hindrance, to form a soluble sandwich complex. The interaction is illustrated by the following equation:



$\text{B}^{\text{in}}\text{Ab}_{(\text{m})}$  = Biotinylated Antibody (Excess Quantity)  
 $\text{Ag}_{\text{PSA}}$  = Native Antigen (Variable Quantity)  
 $\text{Enz}^{\text{Ab}}_{(\text{p})}$  = Enzyme labeled Antibody (Excess Quantity)  
 $\text{Enz}^{\text{Ab}}_{(\text{p})} - \text{Ag}_{\text{PSA}} - \text{B}^{\text{in}}\text{Ab}_{(\text{m})}$  = Antigen-Antibodies Complex  
 $k_a$  = Rate Constant of Association  
 $k_{-a}$  = Rate Constant of Dissociation

Simultaneously, the complex is deposited to the well through the high affinity reaction of streptavidin and biotinylated antibody. This interaction is illustrated below:



After equilibrium is attained, the antibody-bound fraction is separated from unbound antigen by decantation or aspiration. The enzyme activity in the antibody-bound fraction is directly proportional to the native antigen concentration. By utilizing several different serum references of known antigen values, a dose response curve can be generated from which the antigen concentration of an unknown can be ascertained.

**4.0 REAGENTS**

**Materials Provided:**

- A. PSA Calibrators – 1 ml/vial – Icons A-F**  
Six (6) vials of serum references PSA Antigen at levels of 0(A), 5(B), 10(C), 25(D), 50(E) and 100(F) ng/ml. A preservative has been added. Store at 2-8°C.  
**Note:** The calibrators, human serum based, were calibrated using a reference preparation, which was assayed against the 1<sup>st</sup> IS 96/670.
- B. PSA Enzyme Reagent – 13 ml/vial – Icon**   
One (1) vial containing enzyme labeled antibody, biotinylated monoclonal mouse IgG in buffer, dye, and preservative. Store at 2-8°C.
- C. Streptavidin Coated Plate – 96 wells – Icon**   
One 96-well microplate coated with streptavidin and packaged in an aluminum bag with a drying agent. Store at 2-8°C.
- D. Wash Solution Concentrate – 20 ml/vial – Icon**   
One (1) vial containing a surfactant in buffered saline. A preservative has been added. Store at 2-8°C. (see Reagent Preparation Section).
- E. Substrate A – 7 ml/vial – Icon S<sup>A</sup>**  
One (1) vial containing tetramethylbenzidine (TMB) in buffer. Store at 2-8°C.
- F. Substrate B – 7 ml/vial – Icon S<sup>B</sup>**  
One (1) vial containing hydrogen peroxide (H<sub>2</sub>O<sub>2</sub>) in buffer. Store at 2-8°C. (see Reagent Preparation Section).
- G. Stop Solution – 8 ml/vial – Icon**   
One (1) vial containing a strong acid (1N HCl). Store at 2-8°C.

**H. Product Instructions.**  
**Note 1:** Do not use reagents beyond the kit expiration date.  
**Note 2:** Avoid extended exposure to heat and light. **Opened reagents are stable for sixty (60) days when stored at 2-8°C. Kit and component stability are identified on the label.**  
**Note 3:** Above reagents are for a 96-well microplate. For other kit configurations, refer to the table at the end of this insert.

**4.1 Required But Not Provided:**

1. Pipette(s) capable of delivering 0.025, 0.050 & 0.100 ml (25, 50, & 100 µl) volumes with a precision of better than 1.5%.
2. Dispenser(s) for repetitive deliveries of 0.100 & 0.350ml (100 & 350µl) volumes with a precision of better than 1.5%.
3. Microplate washers or a squeeze bottle (optional).
4. Microplate Reader with 450nm and 620nm wavelength absorbance capability.
5. Absorbent Paper for blotting the microplate wells.
6. Plastic wrap or microplate covers for incubation steps.
7. Vacuum aspirator (optional) for wash steps.
8. Timer.

**9. Quality control materials**

**5.0 PRECAUTIONS**

**For In Vitro Diagnostic Use**  
**Not for Internal or External Use in Humans or Animals**

All products that contain human serum have been found to be non-reactive for Hepatitis B Surface Antigen, HIV 1&2 and HCV Antibodies by FDA licensed reagents. Since no known test can offer complete assurance that infectious agents are absent, all human serum products should be handled as potentially hazardous and capable of transmitting disease. Good laboratory procedures for handling blood products can be found in the Center for Disease Control / National Institute of Health, "Biosafety in Microbiological and Biomedical Laboratories," 2nd Edition, 1988, HHS Publication No. (CDC) 88-8395.

**Safe Disposal of kit components must be according to local regulatory and statutory requirement.**

**6.0 SPECIMEN COLLECTION AND PREPARATION**

The specimens shall be blood, serum in type and the usual precautions in the collection of venipuncture samples should be observed. For accurate comparison to established normal values, a fasting morning serum sample should be obtained. The blood should be collected in a plain redtop venipuncture tube without additives or anti-coagulants. Allow the blood to clot. Centrifuge the specimen to separate the serum from the cells.

**In patients receiving therapy with high biotin doses (i.e. >5mg/day), no sample should be taken until at least 8 hours after the last biotin administration, preferably overnight to ensure fasting sample.**

Samples may be refrigerated at 2-8°C for a maximum period of five (5) days. If the specimen(s) cannot be assayed within this time, the sample(s) may be stored at temperatures of -20°C for up to 30 days. Avoid use of contaminated devices. Avoid repetitive freezing and thawing. When assayed in duplicate, 0.050 ml (50 µl) of the specimen is required.

**7.0 QUALITY CONTROL**

Each laboratory should assay controls at levels in the low, normal and elevated range for monitoring assay performance. These controls should be treated as unknowns and values determined in every test procedure performed. Quality control charts should be maintained to follow the performance of the supplied reagents. Pertinent statistical methods should be employed to ascertain trends. Significant deviation from established performance can indicate unnoticed change in experimental conditions or degradation of kit reagents. Fresh reagents should be used to determine the reason for the variations.

**8.0 REAGENT PREPARATION**

1. **Wash Buffer**  
Dilute contents of wash concentrate to 1000ml with distilled or deionized water in a suitable storage container. Store diluted buffer at 2-30°C for up to 60 days.
2. **Working Substrate Solution** – Stable for one year  
Pour the contents of the amber vial labeled Solution 'A' into the clear vial labeled Solution 'B'. Place the yellow cap on the clear vial for easy identification. Mix and label accordingly. Store at 2 - 8°C.

**Note1: Do not use the working substrate if it looks blue.**  
**Note 2: Do not use reagents that are contaminated or have bacteria growth.**

**9.0 TEST PROCEDURE**

*Before proceeding with the assay, bring all reagents, serum reference calibrators and controls to room temperature (20 - 27°C).*

**\*\*Test Procedure should be performed by a skilled individual or trained professional\*\***

1. Format the microplates' wells for each serum reference calibrator, control and patient specimen to be assayed in

duplicate. **Replace any unused microwell strips back into the aluminum bag, seal and store at 2-8°C.**

2. Pipette 0.025ml (25µl) of the appropriate serum reference calibrator, control or specimen into the assigned well.
3. Add 0.100ml (100µl) of the PSA Enzyme Reagent to each well. **It is very important to dispense all reagents close to the bottom of the coated well.**
4. Swirl the microplate gently for 20-30 seconds to mix and cover.
5. Incubate 30 minutes at room temperature.
6. Discard the contents of the microplate by decantation or aspiration. If decanting, tap and blot the plate dry with absorbent paper.
7. Add 0.350ml (350µl) of wash buffer (see Reagent Preparation Section), decant (tap and blot) or aspirate. Repeat two (2) additional times for a total of three (3) washes. **An automatic or manual plate washer can be used. Follow the manufacturer's instruction for proper usage. If a squeeze bottle is employed, fill each well by depressing the container (avoiding air bubbles) to dispense the wash. Decant the wash and repeat two (2) additional times.**
8. Add 0.100ml (100µl) of working substrate solution to all wells (see Reagent Preparation Section). **Always add reagents in the same order to minimize reaction time differences between wells.**  
**DO NOT SHAKE THE PLATE AFTER SUBSTRATE ADDITION**
9. Incubate at room temperature for fifteen (15) minutes.
10. Add 0.050ml (50µl) of stop solution to each well and mix gently for 15-20 seconds. **Always add reagents in the same order to minimize reaction time differences between wells.**
11. Read the absorbance in each well at 450nm (using a reference wavelength of 620-630nm to minimize well imperfections) in a microplate reader. **The results should be read within thirty (30) minutes of adding the stop solution.**

**10.0 CALCULATION OF RESULTS**

A dose response curve is used to ascertain the concentration of PSA in unknown specimens.

1. Record the absorbance obtained from the printout of the microplate reader as outlined in Example 1.
2. Plot the absorbance for each duplicate serum reference versus the corresponding PSA concentration in ng/ml on linear graph paper (do not average the duplicates of the serum references before plotting).
3. Draw the best-fit curve through the plotted points.
4. To determine the concentration of PSA for an unknown, locate the average absorbance of the duplicates for each unknown on the vertical axis of the graph, find the intersecting point on the curve, and read the concentration (in ng/ml) from the horizontal axis of the graph (the duplicates of the unknown may be averaged as indicated). In the following example, the average absorbance (1.142) intersects the dose response curve at (23.6 ng/ml) PSA concentration (See Figure 1).

**Note:** Computer data reduction software designed for ELISA assays may also be used for the data reduction. **If such software is utilized, the validation of the software should be ascertained.**


**EXAMPLE 1**

Sample I.D.	Well Number	Abs (A)	Mean Abs (B)	Value (ng/ml)
Cal A	A1	0.019	0.019	0
	B1	0.019		
Cal B	C1	0.279	0.276	5
	D1	0.273		
Cal C	E1	0.567	0.563	10
	F1	0.559		
Cal D	G1	1.248	1.213	25
	H1	1.179		
Cal E	A2	2.051	1.999	50
	B2	1.947		
Cal F	C2	2.892	2.833	100
	D2	2.775		
Patient	E2	1.186	1.142	23.6

	F2	1.099		
--	----	-------	--	--

\*The data presented in Example 1 and Figure 1 is for illustration only and **should not** be used in lieu of a dose response curve prepared with each assay.

Figure 1

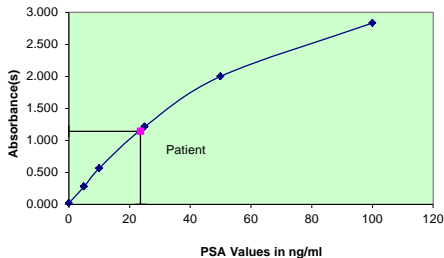

### 11.0 Q.C. PARAMETERS

In order for the assay results to be considered valid the following criteria should be met:

- The absorbance (OD) of calibrator F should be  $\geq 1.3$ .
- Four out of six quality control pools should be within the established ranges.

### 12.0 RISK ANALYSIS

The MSDS and Risk Analysis Form for this product are available on request from Monobind Inc.

#### 12.1 Assay Performance

- It is important that the time of reaction in each well is held constant to achieve reproducible results.
- Pipetting of samples should not extend beyond ten (10) minutes to avoid assay drift.
- Highly lipemic, hemolyzed or grossly contaminated specimen(s) should not be used.
- If more than one (1) plate is used, it is recommended to repeat the dose response curve.
- The addition of substrate solution initiates a kinetic reaction, which is terminated by the addition of the stop solution. Therefore, the substrate and stop solution should be added in the same sequence to eliminate any time-deviation during reaction.
- Plate readers measure vertically. Do not touch the bottom of the wells.
- Failure to remove adhering solution adequately in the aspiration or decantation wash step(s) may result in poor replication and spurious results.
- Use components from the same lot. No intermixing of reagents from different batches.
- Patient specimens with PSA concentrations above 100 ng/ml may be diluted (for example 1/10 or higher) with normal female serum (PSA = 0 ng/ml) and re-assayed. The sample's concentration is obtained by multiplying the result by the dilution factor (10).
- Accurate and precise pipetting, as well as following the exact time and temperature requirements prescribed are essential. Any deviation from Monobind's IFU may yield inaccurate results.
- All applicable national standards, regulations and laws, including, but not limited to, good laboratory procedures, must be strictly followed to ensure compliance and proper device usage.
- It is important to calibrate all the equipment e.g. Pipettes, Readers, Washers and/or the automated instruments used with this device, and to perform routine preventative maintenance.
- Risk Analysis - as required by CE Mark IVD Directive 98/79/EC - for this and other devices, made by Monobind, can be requested via email from [Monobind@monobind.com](mailto:Monobind@monobind.com).

#### 12.2 Interpretation

- Measurements and interpretation of results must be performed by a skilled individual or trained professional.

- Laboratory results alone are only one aspect for determining patient care and should not be the sole basis for therapy, particularly if the results conflict with other determinants.
- The reagents for AccuBind® ELISA procedure have been formulated to eliminate maximal interference; however, potential interactions between rare serum specimens and test reagents can cause erroneous results. Heterophilic antibodies often cause these interactions and have been known to be problems for all kinds of immunoassays (Boscato, LM, Stuart, MC. "Heterophilic antibodies: a problem for all immunoassays" *Clin. Chem.* 1988; 34:27-33). For diagnostic purposes, the results from this assay should be used in combination with clinical examination, patient history and all other clinical findings.
- For valid test results, adequate controls and other parameters must be within the listed ranges and assay requirements.
- If test kits are altered, such as by mixing parts of different kits, which could produce false test results, or if results are incorrectly interpreted, **Monobind shall have no liability**.
- If computer controlled data reduction is used to interpret the results of the test, it is imperative that the predicted values for the calibrators fall within 10% of the assigned concentrations.
- PSA is elevated in benign prostatic hypertrophy (BPH). Clinically, an elevated PSA value alone is not of diagnostic value as a specific test for cancer and should only be used in conjunction with other clinical manifestations (observations) and diagnostic procedures (prostate biopsy). Free PSA determinations may be helpful in regard to the discrimination of BPH and prostate cancer conditions.<sup>5</sup>
- Due to the variation in the calibration used in PSA/ fPSA test kits and differences in epitopic recognition of different antibodies, it is always suggested that the patient sample should be tested with PSA/ fPSA tests made by the same manufacturer. **(Monobind Inc. offers a fPSA ELISA test that should be used for consistency reasons, when needed.)**

### 13.0 PERFORMANCE CHARACTERISTICS

Healthy males are expected to have values below 4 ng/ml.<sup>4</sup>

Healthy Males	<4 ng/ml
---------------	----------

It is important to keep in mind that establishment of a range of values, which can be expected to be found by a given method for a population of "normal"-persons, is dependent upon a multiplicity of factors: the specificity of the method, the population tested and the precision of the method in the hands of the analyst. For these reasons, each laboratory should depend upon the range of expected values established by the Manufacturer only until an in-house range can be determined by the analysts using the method with a population indigenous to the area in which the laboratory is located.

### 14.0 PERFORMANCE CHARACTERISTICS

#### 14.1 Precision

The within and between assay precisions of the PSA AccuBind® ELISA test system were determined by analyses on three different levels of control sera. The number, mean value, standard deviation and coefficient of variation for each of these control sera are presented in Table 2 and Table 3.

Sample	N	X	$\sigma$	C.V.
Level 1	20	1.06	0.06	5.2%
Level 2	20	3.56	0.18	5.1%
Level 3	20	23.07	0.88	3.8%

Sample	N	X	$\sigma$	C.V.
Level 1	20	0.98	0.08	8.5%
Level 2	20	3.35	0.19	5.7%
Level 3	20	23.17	0.95	4.1%

\*As measured in ten experiments in duplicate.

#### 14.2 Sensitivity

The PSA AccuBind® ELISA test system has a sensitivity of 0.0003 ng/well. This is equivalent to a sample containing 0.013 ng/ml PSA concentration.

#### 14.3 Accuracy

The PSA AccuBind® ELISA test system was compared with a reference Elisa method. Biological specimens from low, normal, and elevated concentrations were assayed. The total number of such specimens was 241. The least square regression equation and the correlation coefficient were computed for the PSA AccuBind® ELISA test method in comparison with the reference method. The data obtained is displayed in Table 4.

Method	Mean	Least Square Regression Analysis	Correlation Coefficient
This Method (X)	5.62	$y = -0.0598 + 0.98(X)$	0.987
Reference (Y)	5.57		

Only slight amounts of bias between the PSA AccuBind® ELISA test system and the reference method are indicated by the closeness of the mean values. The least square regression equation and correlation coefficient indicates excellent method agreement.

#### 14.4 Specificity:

No interference was detected with the performance of PSA AccuBind® ELISA test system upon addition of massive amounts of the following substances to a human serum pool.

Substance	Concentration
Acetylsalicylic Acid	100 µg/ml
Ascorbic Acid	100 µg/ml
Caffeine	100 µg/ml
CEA	10 µg/ml
AFP	10 µg/ml
CA-125	10,000 U/ml
hCG	1000 IU/ml
hLH	10 IU/ml
hTSH	100 mIU/ml
hPRL	100 µg/ml

### 15.0 REFERENCES

- Christensson A, Laurell CB, Lilja H, *Eur J Biochem*, 194, 755-63 (1990).
- Watt KW, et al., *Proc Nat Acad Sci USA*, 83, 3166-70 (1986).
- Chen Z, Prestigiacomo A, Stamey T, *Clin Chem*, 41, 1273-82 (1995).
- Wild D, *The Immunoassay Handbook*, Stockton Press, 452, (1994).
- Junker R, Brandt B, Zechel C, Assmann G, *Clin Chem*, 43, 1588-94 (1997).
- Prestigiacomo AF, Stamey TA, "Physiological variations of serum prostate antigen in the (4-10 ng/ml) range in male volunteers", *J Urol*, 155, 1977-80 (1996).
- Stamey TA, McNeal JE, Yemoto CM, Sigal BM, Johnstone IM, "Biological determinants of cancer progression in men with prostate cancer", *JAMA* 281, 1395-1400 (1999).
- Chen Z, Prestigiacomo A, Stamey T, "Purification and characterization of Prostate Specific Antigen (PSA) Complexed to  $\alpha_1$ - Anticymotrypsin: Potential reference Material for International Standardization of PSA Immunoassays", *Clin Chem*, 41/9, 1273-1282 (1995).
- Horton GL, Bahnson RR, Datt M, Cfhon KM, Catalona WJ and Landenson JH, "Differences in values obtained with two assays of Prostate Specific Antigen", *J Urol*, 139, 762-72 (1988).
- Stenman UH, Leinonen J, Alfthan H, Rannikko S, Tuhkanen K and Alfthan O, "A complex between prostate specific antigen and  $\alpha_1$ -anticymotrypsin is the major form of prostate specific antigen in serum of patients with prostate cancer: assay of complex improves clinical sensitivity for cancer", *Cancer Res*, 51, 222-26 (1991).

Revision: 6 Date: 2022-MAY-01 DCO: 1557  
MP2125 Product Code: 2125-300

Size	96(A)	192(B)
Reagent (fill)	A) 1ml set	1ml set
	B) 1 (13ml)	2 (13ml)
	C) 1 plate	2 plates
	D) 1 (20ml)	1 (20ml)
	E) 1 (7ml)	2 (7ml)
	F) 1 (7ml)	2 (7ml)
	G) 1 (8ml)	2 (8ml)

For Orders and Inquires, please contact

**Monobind Inc.**  
100 North Pointe Drive  
Lake Forest, CA 92630 USA

Tel: +1 949.951.2665 Mail: [info@monobind.com](mailto:info@monobind.com)  
Fax: +1 949.951.3539 Fax: [www.monobind.com](http://www.monobind.com)



Please visit our website to learn more about our products and services.

### Glossary of Symbols (EN 980/ISO 15223)

