



**Free  $\beta$ -Subunit Human Chorionic Gonadotropin (Free Beta hCG) Test System**  
**Product Code: 2025-300**

**1.0 INTRODUCTION**

Intended Use: The Quantitative Determination of Free Beta ( $\beta$ ) Chorionic Gonadotropin Subunit Concentration in Human Serum by a Microplate Enzyme Immunoassay, Colorimetric

**2.0 SUMMARY AND EXPLANATION OF THE TEST**

Human chorionic gonadotropin (hCG) concentration increases dramatically in blood and urine during normal pregnancy. hCG is secreted by placental tissue, beginning with the primitive trophoblast, almost from the time of implantation, and serves to support the corpus luteum during the early weeks of pregnancy. hCG or hCG similar glycoproteins can also be produced by a wide variety of trophoblastic and nontrophoblastic tumors. The measurement of hCG, by assay systems with suitable sensitivity and specificity has proven great value in the detection of pregnancy and the potential diagnosis of early pregnancy disorders. Free  $\beta$ -subunit hCG testing has improved the diagnostic probability of abnormal pregnancy/disease states.<sup>1</sup>

Patients with trophoblastic diseases produce ordinary and irregular forms of hCG; e.g. nicked hCG, hCG missing the  $\beta$ -subunit C-terminal segment, hyperglycosylated hCG and free  $\beta$  subunit. On the other hand, common epithelial tumors of the urogenital tract frequently express the free  $\beta$ -Subunit of hCG with no concomitant expression of its heterodimer partner, the common  $\alpha$ -subunit of the glycoprotein hormone. While most hCG assays do a very good job of monitoring the normal pregnancies, still there needs to be a system of differential diagnosis of ovarian tumors, epithelial tumors and trophoblastic malfunctions. That is where determination of free  $\alpha$ -subunit, free  $\beta$ -subunit, nicked hCG and nonnicked hCG etc are of individual value.

Although Free  $\beta$ -Subunit hCG normally constitutes less than 1% of the total hCG concentrations in normal pregnancy, it constitutes a significant part (as much as 26% of hCG) in trophoblast disease.<sup>2,3</sup> There is also increasing evidence that free beta subunit may be better than total hCG measurement in assessing Down's Syndrome.<sup>4</sup>

In this method, Free Beta hCG calibrator, patient specimen or control is first added to an anti-Free Beta hCG coated well. Assay Buffer is added and the reactants mixed. Reaction between the antibody and native Free Beta hCG forms complex that binds with the antibodies coated to the well. The excess serum proteins are washed away via a wash step. Another enzyme labeled monoclonal antibody specific to Free Beta hCG is added to the wells. The enzyme labeled antibody binds to the Free Beta hCG already immobilized on the well. Excess enzyme is washed off via a wash step. A color is generated by the addition of a substrate. The intensity of the color generation is directly proportional to the concentration of the Free Beta hCG in the sample.


The employment of several serum references of known Free Beta Chorionic Gonadotropin levels permits the construction of a dose response curve of activity and concentration. From comparison to the dose response curve, an unknown specimen's activity can be correlated with Free Beta hCG concentration.

**3.0 PRINCIPLE**

**Immunoenzymometric sequential assay (TYPE 4):**


The essential reagents required for an immunoenzymometric assay include high affinity and specificity antibodies (enzyme and immobilized), with different and distinct epitope recognition, in excess, and native antigen.

Upon mixing assay buffer and a serum containing the native antigen, reaction results between the native antigen and the coated antibody, forming an antibody-antigen complex. This interaction is illustrated below:



$Ab_{(c)}$  = Coated Antibody (Excess Quantity)  
 $Ag$  = Native Antigen (Variable Quantity)  
 $AgAb_{(c)}$  = Antigen-Antibody complex (Variable Quant.)  
 $k_a$  = Rate Constant of Association  
 $k_{-a}$  = Rate Constant of Disassociation

After a suitable incubation period, the antibody-antigen bound fraction is separated from unbound antigen by decantation or aspiration. Another antibody (directed at a different epitope) labeled with an enzyme is added. Another interaction occurs to form an enzyme labeled antibody-antigen-biotinylated-antibody complex on the surface of the wells.



$EnzAb$  = Enzyme labeled Antibody (Excess Quantity)  
 $k_b$  = Rate Constant of Association  
 $k_{-b}$  = Rate Constant of Disassociation

Excess enzyme is washed off via a wash step. A suitable substrate is added to produce color measurable with the use of a microplate spectrophotometer. The enzyme activity on the well is directly proportional to the native free antigen concentration. By utilizing several different serum references of known antigen concentration, a dose response curve can be generated from which the antigen concentration of an unknown can be ascertained.

**4.0 REAGENTS**

**Materials Provided:**

- A. Free Beta hCG Calibrators – 1 ml/vial - Icons A-F**  
Six (6) vials of references  $\beta$ -hCG Antigen at levels of 0(A), 10(B), 25(C), 50(D), 100(E) and 250(F) ng/ml. Store at 2-8°C. A preservative has been added.
- Note:** The calibrators, human serum based, were calibrated using a reference preparation, which was assayed against the WHO 1<sup>st</sup> IRP (75/551).
- Conversion to mass units =** One (1) mIU/ml is equivalent to 1 ng/ml
- B. Assay Buffer – 7 ml/vial - Icon B**  
One (1) vial containing buffer, dye, surfactants and preservatives. Store at 2-8°C.
- C. Free Beta hCG Enzyme Reagent – 13 ml/vial - Icon C**  
One (1) vial containing Enzyme (HRP) labeled monoclonal mouse IgG in buffer, dye, and preservative. Store at 2-8°C.
- D. Free Beta hCG Antibody Coated Plate – 96 wells - Icon D**  
One 96-well microplate coated with anti- $\beta$ hCG mouse IgG and packaged in an aluminum bag with a drying agent. Store at 2-8°C.
- E. Wash Solution Concentrate – 20 ml/vial - Icon E**  
One (1) vial containing a surfactant in buffered saline. A preservative has been added. Store at 2-8°C.
- F. Substrate A – 7 ml/vial - Icon S<sup>A</sup>**  
One (1) vial containing tetramethylbenzidine (TMB) in buffer. Store at 2-8°C.
- G. Substrate B – 7 ml/vial - Icon S<sup>B</sup>**

One (1) vial containing hydrogen peroxide (HB<sub>26</sub>OB<sub>26</sub>) in buffer. Store at 2-8°C.

**H. Stop Solution – 8 ml/vial - Icon H**

One (1) vial containing a strong acid (1N HCl). Store at 2-8°C.

**I. Product Instructions.**

- Note 1:** Do not use reagents beyond the kit expiration date.
- Note 2:** Opened reagents are stable for sixty (60) days when stored at 2-8°C. **Opened reagents are stable for sixty (60) days when stored at 2-8°C. Kit and component stability are identified on the label.**
- Note 3:** Above reagents are for a single 96-well microplate. For other kit configurations, refer to table at the end of the instructions.

**4.1 Required But Not Provided:**

- 1. Pipette capable of delivering 0.025ml (25 $\mu$ l), 0.050ml (50 $\mu$ l) 0.100 ml (100  $\mu$ l) volumes with a precision of better than 1.5%.
- 2. Dispenser(s) for repetitive deliveries of 0.50 ml (50  $\mu$ l), 0.100 ml (100  $\mu$ l) and 0.350 ml (0.350  $\mu$ l) volumes with a precision of better than 1.5%.
- 3. Microplate washers or a squeeze bottle (optional).
- 4. Microplate Reader with 450nm and 620nm wavelength absorbance capability.
- 5. Absorbent Paper for blotting the microplate wells.
- 6. Plastic wrap or microplates cover for incubation steps.
- 7. Vacuum aspirator (optional) for wash steps.
- 8. Timer.
- 9. Quality control materials.

**5.0 PRECAUTIONS**

**For In Vitro Diagnostic Use  
 Not for Internal or External Use in Humans or Animals**

All products that contain human serum have been found to be non-reactive for Hepatitis B Surface Antigen, HIV 1&2 and HCV Antibodies by FDA licensed reagents. Since no known test can offer complete assurance that infectious agents are absent, all human serum products should be handled as potentially hazardous and capable of transmitting disease. Good laboratory procedures for handling blood products can be found in the Center for Disease Control / National Institute of Health, "Biosafety in Microbiological and Biomedical Laboratories," 2nd Edition, 1988, HHS Publication No. (CDC) 88-8395.

**Safe Disposal of kit components must be according to local regulatory and statutory requirement.**

**6.0 SPECIMEN COLLECTION AND PREPARATION**

The specimens shall be blood serum in type and the usual precautions in the collection of venipuncture samples should be observed. For accurate comparison to established normal values, a fasting morning serum sample should be obtained. The blood should be collected in a plain redtop venipuncture tube without additives or anti-coagulants. Allow the blood to clot for samples. Centrifuge the specimen to separate the serum from the cells.

Samples may be refrigerated at 2-8°C for a maximum period of five (5) days. If the specimen(s) cannot be assayed within this time, the sample(s) may be stored at temperatures of -20°C for up to 30 days. Avoid use of contaminated devices. Avoid repetitive freezing and thawing. When assayed in duplicate, 0.050 ml (50  $\mu$ l) of the specimen is required.

**7.0 QUALITY CONTROL**

Each laboratory should assay controls at levels in the low, medium and high ranges of the dose response curve for monitoring assay performance. These controls should be treated as unknowns and values determined in every test procedure performed. Quality control charts should be maintained to follow the performance of the supplied reagents. Pertinent statistical methods should be employed to ascertain trends. Significant deviation from established performance can indicate unnoticed change in experimental conditions or degradation of kit reagents. Fresh reagents should be used to determine the reason for the variations.

**8.0 REAGENT PREPARATION**

- 1. **Wash Buffer**  
Dilute contents of wash concentrate to 1000ml with distilled or deionized water in a suitable storage container. Store diluted buffer at 2-30°C for up to 60 days.
- 2. **Working Substrate Solution** – Stable for one (1) year  
Pour the contents of the amber vial labeled Solution 'A' into the clear vial labeled Solution 'B'. Place the yellow cap on the clear vial for easy identification. Mix and label accordingly. Store at 2 - 8°C.

**Note 1: Do not use the working substrate if it looks blue.  
 Note 2: Do not use reagents that are contaminated or have bacteria growth.**

**9.0 TEST PROCEDURE**

*Before proceeding with the assay, bring all reagents, serum reference calibrators and controls to room temperature (20-27°C).  
 \*\*Test Procedure should be performed by a skilled individual or trained professional\*\**

- 1. Format the microplates' wells for each serum reference, control and patient specimen to be assayed in duplicate. **Replace any unused microwell strips back into the aluminum bag, seal and store at 2-8°C.**
- 2. Pipette 0.025 ml (25  $\mu$ l) of the appropriate serum reference, control or specimen into the assigned well.
- 3. Add 0.050ml of Assay Buffer to each well. **It is very important to dispense all reagents close to the bottom of the coated well.**
- 4. Swirl the microplate gently for 20-30 seconds to mix and cover.
- 5. Incubate 30 minutes at room temperature.
- 6. Discard the contents of the microplate by decantation or aspiration. If decanting, tap and blot the plate dry with absorbent paper.
- 7. Add 0.350 ml (350  $\mu$ l) of wash buffer (see Reagent Preparation section), decant (tap and blot) or aspirate. Repeat two (2) additional times for a total of three (3) washes. **An automatic or manual plate washer can be used. Follow the manufacturer's instruction for proper usage. If a squeeze bottle is employed, fill each well by depressing the container (avoiding air bubbles) to dispense the wash. Decant the wash and repeat two (2) additional times.**
- 8. Add 0.100 ml (100  $\mu$ l) of the Free Beta hCG Enzyme Reagent to each well.  
**DO NOT SHAKE THE PLATE AFTER ENZYME ADDITION**
- 9. Cover and incubate 15 minutes at room temperature.
- 10. Discard the contents of the microplate by decantation or aspiration. If decanting, blot the plate dry with absorbent paper.
- 11. Add 0.350 ml (350  $\mu$ l) of wash buffer (see Reagent Preparation Section), decant (tap and blot) or aspirate. Repeat two (2) additional times for a total of three (3) washes. **An automatic or manual plate washer can be used. Follow the manufacturer's instruction for proper usage. If a squeeze bottle is employed, fill each well by depressing the container (avoiding air bubbles) to dispense the wash. Decant the wash and repeat two (2) additional times.**
- 12. Add 0.100 ml (100  $\mu$ l) of working substrate solution to all wells (see Reagent Preparation Section). **Always add reagents in the same order to minimize reaction time differences between wells.**  
**DO NOT SHAKE PLATE AFTER SUBSTRATE ADDITION**
- 13. Incubate at room temperature for fifteen (15) minutes.
- 14. Add 0.050 ml (50  $\mu$ l) of stop solution to each well and mix gently for 15-20 seconds. **Always add reagents in the same order to minimize reaction time differences between wells.**
- 15. Read the absorbance in each well at 450nm (using a reference wavelength of 620-630nm to minimize well imperfections) in a microplate reader. **The results should be read within thirty (30) minutes of adding the stop solution.**

**10.0 CALCULATION OF RESULTS**

A dose response curve is used to ascertain the concentration of Free Beta hCG in unknown specimens.  
 1. Record the absorbance obtained from the printout of the microplate reader as outlined in Example 1.

- Plot the absorbance for each duplicate serum reference versus the corresponding Free Beta hCG concentration in ng/ml on linear graph paper (do not average the duplicates of the serum references before plotting).
- Draw the best-fit curve through the plotted points.
- To determine the concentration of Free Beta hCG for an unknown, locate the average absorbance of the duplicates for each unknown on the vertical axis of the graph, find the intersecting point on the curve, and read the concentration (in ng/ml) from the horizontal axis of the graph (the duplicates of the unknown may be averaged as indicated). In the following example, the average absorbance (0.366) intersects the dose response curve at 14.7 ng/ml Free Beta hCG concentration (See Figure 1).


**Note:** Computer data reduction software designed for ELISA assays may also be used for the data reduction. If such software is utilized, the validation of the software should be ascertained.

#### EXAMPLE 1

Sample I.D.	Well Position	Abs (A)	Mean Abs (B)	Value (ng/ml)
Cal A	A1	0.008	0.008	0
	B1	0.008		
Cal B	C1	0.290	0.266	10
	D1	0.242		
Cal C	E1	0.557	0.536	25
	F1	0.513		
Cal D	G1	1.021	0.984	50
	H1	0.946		
Cal E	A2	1.695	1.662	100
	B2	1.630		
Cal F	C2	2.910	2.803	250
	D2	2.695		
Control	E2	1.414	1.343	79.4
	F2	1.271		
Patient	G2	0.362	0.366	14.7
	H2	0.370		

\*The data presented in Example 1 and Figure 1 is for illustration only and **should not** be used in lieu of a dose response curve prepared with each assay.

Figure 1

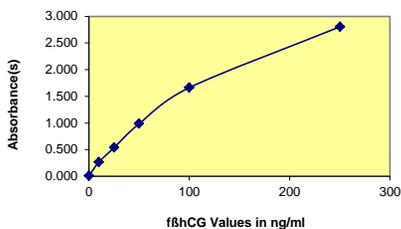

### 11.0 Q.C. PARAMETERS

In order for the assay results to be considered valid the following criteria should be met:

- Maximum Absorbance (Calibrator 'F') = >1.3
- Maximum Absorbance (Calibrator 'A') =  $U \leq U \cdot 0.1$
- Four out of six quality control pools should be within the established ranges.

### 12.0 RISK ANALYSIS

The MSDS and Risk Analysis Form for this product are available on request from Monobind Inc.

#### 12.1 Assay Performance

- It is important that the time of reaction in each well is held constant to achieve reproducible results.
- Pipetting of samples should not extend beyond ten (10) minutes to avoid assay drift.
- The reagents for the test system procedures have been formulated to eliminate maximal interference; however, potential interaction between rare serum specimens and test reagents can cause erroneous results. Heterophilic antibodies often cause these interactions and have been known to be problems for all kinds of immunoassays (Boscato LM, Stuart MC. "Heterophilic antibodies: a problem for all immunoassays" *Clin.Chem.* 1988:3427-33). For diagnostic purposes, the results from this assay should be used in combination with clinical examination, patient history and all other clinical findings.
- Highly lipemic, hemolyzed or grossly contaminated specimen(s) should not be used.
- If more than one (1) plate is used, it is recommended to repeat the dose response curve.
- The addition of substrate solution initiates a kinetic reaction, terminated by the addition of the stop solution. Therefore, the substrate and stop solution should be added in the same sequence to eliminate any time-deviation during reaction.
- Plate readers measure vertically. Do not touch the bottom of the wells.
- Failure to remove adhering solution adequately in the aspiration or decantation wash step(s) may result in poor replication and spurious results.
- Use components from the same lot. No intermixing of reagents from different batches.
- Patient specimens with Free Beta hCG concentrations above 50 ng/ml may be diluted (for example 1/10) with normal male serum (Free Beta hCG < 1 ng/ml) and re-assayed. The sample's concentration is obtained by multiplying the result by the dilution factor.
- Accurate and precise pipetting, as well as following the exact time and temperature requirements prescribed are essential. Any deviation from Monobind's IFU may yield inaccurate results.
- All applicable national standards, regulations and laws, including, but not limited to, good laboratory procedures, must be strictly followed to ensure compliance and proper device usage.
- It is important to calibrate all the equipment e.g. Pipettes, Readers, Washers and/or the automated instruments used with this device, and to perform routine preventative maintenance.
- Risk Analysis- as required by CE Mark IVD Directive 98/79/EC - for this and other devices, made by Monobind, can be requested via email from [Monobind@monobind.com](mailto:Monobind@monobind.com).

#### 12.2 Interpretation

- Measurements and interpretation of results must be performed by a skilled individual or trained professional.**
- Laboratory results alone are only one aspect for determining patient care and should not be the sole basis for therapy, particularly if the results conflict with other determinants.
- The reagents for AccuBind® ELISA procedures have been formulated to eliminate maximal interference; however, potential interaction between rare serum specimens and test reagents can cause erroneous results. Heterophilic antibodies often cause these interactions and have been known to be problems for all kinds of Immunoassays (Boscato LM, Stuart MC "Heterophilic antibodies: a problem for all immunoassays" *Clin. Chem* (1988:3427-33). For diagnostic purposes, the results from this assay should be in combination with clinical examination, patient history, and all other clinical findings.
- For valid test results, adequate controls and other parameters must be within the listed ranges and assay requirements.
- If test kits are altered, such as by mixing parts of different kits, which could produce false test results, or if results are incorrectly interpreted, **Monobind shall have no liability.**
- If computer controlled data reduction is used to interpret the results of the test, it is imperative that the predicted values for the calibrators fall within 10% of the assigned concentrations.

### 13.0 EXPECTED RANGES OF VALUES

Serum Free beta hCG (as intact hCG) increases rapidly in normal pregnancy reaching maximum levels of approximately 60ng/ml (which is equivalent to 60 mIU/ml) at eight-nine weeks of gestation. This is followed by a gradual decline during the next

eleven to twelve weeks. The ratio of Free Beta hCG to intact hCG reaches 1% at five weeks of pregnancy and remains constant at approximately 0.5% (w/w) for the remaining twenty-two weeks.<sup>2</sup>

The use of Free Beta hCG in combination with AFP levels as a screening protocol for Down syndrome (Trisomy 21) has been promoted to achieve high detection efficiency with low false positive rates.<sup>2</sup>

It is important to keep in mind that establishment of a range of values, which can be expected to be found by a given method for a population of "normal" persons, is dependent upon a multiplicity of factors: the specificity of the method, the population tested and the precision of the method in the hands of the analyst. For these reasons, each laboratory should depend upon the range of expected values established by the Manufacturer only until an in-house range can be determined by the analysts using the method with a population indigenous to the area in which the laboratory is located.

### 14.0 PERFORMANCE CHARACTERISTICS

#### 14.1 Precision

The within and between assay precisions of the Free Beta hCG AccuBind® ELISA test system were determined by analyses on three different levels of control sera. The number, mean value, standard deviation and coefficient of variation for each of these control sera are presented in Table 3 and Table 4.

Sample	N	X	σ	C.V.
Level 1	20	3.5	0.15	4.3%
Level 2	20	10.5	0.55	5.2%
Level 3	20	49.6	1.50	3.0%

Sample	N	X	σ	C.V.
Level 1	10	3.1	0.17	5.5%
Level 2	10	11.2	0.71	6.3%
Level 3	10	48.5	1.75	3.6%

\*As measured in ten experiments in duplicate.

#### 14.2 Sensitivity

The Free Beta hCG AccuBind® ELISA test system has a sensitivity of 0.0007 mIU. This is equivalent to a sample containing 0.026 ng/ml Free Beta hCG concentration.

#### 14.3 Specificity

The cross-reactivity of the Free Beta hCG AccuBind® ELISA test method to selected substances was evaluated by adding the interfering substance to a serum matrix at various concentrations. The cross-reactivity was calculated by deriving a ratio between dose of interfering substance to dose of Chorionic Gonadotropin needed to produce the same absorbance.

Substance	Cross Reactivity
fβ-hCG subunit	1.0000
Intact Chorionic Gonadotropin (hCG)	< 0.0001
Follicle Stimulating Hormone (FSH)	< 0.0001
Luteinizing Hormone (LH)	< 0.0001
Thyroid Stimulating Hormone (TSH)	< 0.0001

### 15.0 REFERENCES

- Henry JB, *Clinical Diagnosis and Management by Laboratory Methods*, WB Saunders Company, 486 (1996).
- Osturk M, et al, *Endocrinology*, 120, 549 (1987).
- Cole LA, et al, *Serono Symposia Publ*, 65, 59-78 (1989).
- Macri JN, and Spencer K, *Am J Obstet Gynecol*, 174, 1668-69 (1996).
- Macri JN, et al, *Am J Obstet Gynecol*, 163, 1248 (1990).
- Cole LA, "β core fragment (β-core, UGP or UGF)", *Tumor Marker Update*, 6, 69-75 (1994).
- Yamanaka N, Kawabata G, Morisue K, Hazama M, Nishimura R, "Urinary hCG β-core fragment as a tumor marker for bladder cancer", *Nippon Hinyokika Gakkai Zasshi*, 84, 700-706 (1993).

- Kinugasa M, Nishimura R, Hasegawa K, Okamura M, Kimura A, Ohtsu F, "Assessment of urinary β-core fragment of hCG as a tumor marker of cervical cancer", *Acta Obstet Gynecol Jpn*, 11, 188-94 (1992).
- Cole LA, "Stability of hCG free β-subunit in urine", *Prenat Diagnosis*, 17, 185-89 (1996).
- Sancken U, Bahner D, "The effect of thermal instability of intact human chorionic gonadotropin on the application of its free β-subunit as a serum marker of Down's syndrome screening", *Prenat Diagnosis*, 15, 731-738 (1995).
- Javadpour N, "Current status of tumor markers in testicular cancer", *Eur Urol*, 21, 34-36 (1992).
- Canick JA, Kellner DN Jr, Palomaki GE, Walker RP, Osathanondh R, "Second trimester levels of maternal urinary gonadotropin peptide in Down syndrome pregnancy", *Prenat Diagnosis*, 15, 752-759 (1995).


Effective Date: 2022-Mar-30 Rev. 2 2022-03-29 DCO: 1543  
MP2025 Product Code: 2025-300

Size	96(A)		192(B)	
	Reagent (fill)	A)	1ml set	1ml set
	B)	1 (7ml)	2 (7ml)	
	C)	1 (13ml)	2 (13ml)	
	D)	1 plate	2 plates	
	E)	1 (20ml)	1 (20ml)	
	F)	1 (7ml)	2 (7ml)	
	G)	1 (7ml)	2 (7ml)	
	H)	1 (8ml)	2 (8ml)	

For Orders and Inquires, please contact

**Monobind Inc.**  
100 North Pointe Drive  
Lake Forest, CA 92630 USA

Tel: +1 949.951.2665 Mail: [info@monobind.com](mailto:info@monobind.com)  
Fax: +1 949.951.3539 Fax: [www.monobind.com](http://www.monobind.com)



CEpartner4U, Eindhovenlaan 13  
3951 DBMaarn, The Netherlands  
[www.cepartner4u.eu](http://www.cepartner4u.eu)

Please visit our website to learn more about our products and services.

### Glossary of Symbols (EN 980/ISO 15223)

